



## Head models of healthy and depressed adults for simulating the electric fields of non-invasive electric brain stimulation

Boayue, Nya Mehnwolo; Csifcsák, Gábor; Puonti, Oula; Thielscher, Axel; Mittner, Matthias

*Published in:*  
F1000Research

*Link to article, DOI:*  
[10.12688/f1000research.15125.2](https://doi.org/10.12688/f1000research.15125.2)

*Publication date:*  
2018

*Document Version*  
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

*Citation (APA):*  
Boayue, N. M., Csifcsák, G., Puonti, O., Thielscher, A., & Mittner, M. (2018). Head models of healthy and depressed adults for simulating the electric fields of non-invasive electric brain stimulation. *F1000Research*, 7, [704]. <https://doi.org/10.12688/f1000research.15125.2>

---

### General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.



## DATA NOTE

# **REVISED** Head models of healthy and depressed adults for simulating the electric fields of non-invasive electric brain stimulation [version 2; referees: 2 approved]

Previously titled: Head models of healthy and depressed adults for simulating the effects of non-invasive brain stimulation

Nya Mehnwolo Boayue <sup>1</sup>, Gábor Csifcsák <sup>1</sup>, Oula Puonti <sup>2,3</sup>, Axel Thielscher <sup>2,3</sup>, Matthias Mittner <sup>1</sup>

<sup>1</sup>Department of Psychology, Faculty of Health Sciences, University of Tromsø - The Arctic University of Norway, Tromsø, 9037, Norway

<sup>2</sup>Center for Magnetic Resonance, Department of Electrical Engineering, Technical University of Denmark, Kongens Lyngby, 2800, Denmark

<sup>3</sup>Danish Research Centre for Magnetic Resonance, Centre for Functional and Diagnostic Imaging and Research, Copenhagen University Hospital, Hvidovre, 2650, Denmark

**v2** First published: 06 Jun 2018, 7:704 (<https://doi.org/10.12688/f1000research.15125.1>)

Latest published: 15 Nov 2018, 7:704 (<https://doi.org/10.12688/f1000research.15125.2>)

## Abstract

During the past decade, it became clear that the electric field elicited by non-invasive brain stimulation (NIBS) techniques such as transcranial direct current stimulation (tDCS) and transcranial magnetic stimulation (TMS) are substantially influenced by variations in individual head and brain anatomy. In addition to structural variations in the healthy, several psychiatric disorders are characterized by anatomical alterations that are likely to further constrain the intracerebral effects of NIBS. Here, we present high-resolution realistic head models derived from structural magnetic resonance imaging data of 19 healthy adults and 19 patients diagnosed with major depressive disorder (MDD). By using a freely available software package for modelling the electric fields induced by different NIBS protocols, we show that our head models are well-suited for assessing inter-individual and between-group variability in the magnitude and focality of tDCS-induced electric fields for two protocols targeting the left dorsolateral prefrontal cortex.

## Keywords

transcranial direct current stimulation (tDCS), transcranial magnetic stimulation (TMS), non-invasive brain stimulation (NIBS), major depressive disorder (MDD), Head models, computational modelling, magnetic resonance imaging (MRI), volume conduction model

## Open Peer Review

Referee Status:

	Invited Referees	
	1	2
<b>REVISED</b>		
<b>version 2</b> published 15 Nov 2018		 report
<b>version 1</b> published 06 Jun 2018	 report	  report

1 **Ilkka Laakso** , Aalto University, Finland

2 **Yu Huang** , New York City, USA

## Discuss this article

Comments (0)

**Corresponding author:** Matthias Mittner ([matthias.mittner@uit.no](mailto:matthias.mittner@uit.no))

**Author roles:** **Boayue NM:** Conceptualization, Data Curation, Formal Analysis, Investigation, Methodology, Software, Validation, Visualization, Writing – Original Draft Preparation; **Csifcsák G:** Conceptualization, Data Curation, Investigation, Methodology, Supervision, Validation, Writing – Original Draft Preparation; **Puonti O:** Data Curation, Formal Analysis, Methodology, Software, Validation, Writing – Review & Editing; **Thielscher A:** Data Curation, Formal Analysis, Methodology, Software, Validation, Writing – Review & Editing; **Mittner M:** Conceptualization, Data Curation, Formal Analysis, Funding Acquisition, Investigation, Methodology, Project Administration, Resources, Software, Supervision, Validation, Visualization, Writing – Original Draft Preparation, Writing – Review & Editing

**Competing interests:** No competing interests were disclosed.

**Grant information:** This work was supported by the Northern Norway Regional Health Authority (grant no. PFP1237-15) for G.Cs. and M.M. and by the Lundbeck foundation (grant no. R118-A11308) and the Novonordisk foundation (grant no. NNF14OC0011413) for O.P. and A.T. The publication charges for this article have been funded by a grant from the publication fund of UiT The Arctic University of Norway. *The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.*

**Copyright:** © 2018 Boayue NM *et al.* This is an open access article distributed under the terms of the [Creative Commons Attribution Licence](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

**How to cite this article:** Boayue NM, Csifcsák G, Puonti O *et al.* **Head models of healthy and depressed adults for simulating the electric fields of non-invasive electric brain stimulation [version 2; referees: 2 approved]** *F1000Research* 2018, 7:704 (<https://doi.org/10.12688/f1000research.15125.2>)

**First published:** 06 Jun 2018, 7:704 (<https://doi.org/10.12688/f1000research.15125.1>)

**REVISED Amendments from Version 1**

We clarified the pipeline for head model creation. Based on the reviewers' comments, we highlighted some additional limitations about the utility of the head models, we added 'electric' and changed 'effects' to 'electric fields' in the title of the manuscript and elaborated a little more on the group differences in tDCS-induced electric fields between MDD and healthy subjects. We also now provide new scripts compatible with the latest released version of SimNIBS (version 2.1.1) for automated simulation of tDCS-induced electric fields.

See referee reports

## Introduction

Non-invasive brain stimulation (NIBS) techniques such as transcranial direct current stimulation (tDCS) and transcranial magnetic stimulation (TMS) have been used to investigate the relationship between activity in different cortical regions and cognitive processes<sup>1,2</sup>. A key advantage of NIBS is that it allows direct manipulation of neural excitability<sup>3</sup>. Therefore when used carefully, it allows causal interpretation of how specific brain regions might be involved in mental phenomena such as perception<sup>4</sup>, working memory<sup>5</sup>, attention<sup>6</sup>, decision-making<sup>7</sup> or emotional regulation<sup>8</sup>. In addition, NIBS has been used as a clinical tool to obtain symptom reduction in several neurological and psychiatric conditions<sup>9–12</sup>. Importantly, the same stimulation protocol can result in different neural effects across individuals because the distribution of stimulation-induced electric fields (E-fields) in the brain is strongly contingent on anatomical variability<sup>13,14</sup>. This can manifest in strong variability in the effects of NIBS on cognitive performance in healthy individuals (e.g., working memory<sup>15,16</sup>) and on treatment outcomes in patients (e.g., depression<sup>17–21</sup>).

Given the heterogeneity in the efficacy of NIBS protocols in modulating behavior and clinical symptoms, there has been a move towards computational modelling of the spatial distribution of E-fields in the brain to understand how stimulation parameters such as electrode placement, electrode rotation or electrode type affects current flow in the neural tissue. After an initial phase during which simplistic spherical head models were used<sup>22</sup>, the focus has shifted to very detailed, realistic head models created from individual structural magnetic resonance (MR) images using freely available tools (e.g. SimNIBS<sup>23</sup> or ROAST<sup>24</sup>). Creating individual head models remains challenging, however, due to (1) the requirement of high-quality structural MR images for each study participant and (2) the need to manually improve the automatic segmentation of the MR images into the different tissue types (i.e., bone, cerebrospinal fluid, white and grey matter, air, etc). As a consequence, individual head models are rarely used in practice. Instead, researchers usually rely on E-fields induced in a reference individual which is generalized to all participants. This approach, of course, neglects the importance of individual brain anatomy which can have strong influences on E-field distribution<sup>13</sup>.

To circumvent this issue, the New York (NY) Head model<sup>25</sup> was created from the ICBM152 (v6 template<sup>26,27</sup> and v2009b template<sup>28</sup>), which is a non-linear average of 152 individual MRIs

and is extended to the full head and neck region by fusing it with an average of an additional 26 brains. Therefore, this head model represents an unbiased population average and should be a better representation of the individual participants than any randomly picked reference individual. However, calculation of the electric field on a single head model does not allow to quantify variation across individuals that can be substantial both in cortical regions directly below the electrodes and those that are farther away from the stimulation sites. Also, given that the NY Head was created using healthy individuals, possible systematic differences between patient groups may not be noticed.

To improve this situation, we present 38 head models created from MR images of 19 healthy participants and 19 patients with major depressive disorder (MDD). These head models were manually checked and edited to improve their accuracy in giving a faithful representation of cortical regions. Our head models can aid future research in at least three ways: First, calculating electric fields across a large sample allows to get a sense of the variability of the induced E-field due to anatomical differences. Second, our head models also enable comparison of the neural effects on NIBS protocols in healthy vs. depressed brains. Given the different protocols used for left dorsolateral prefrontal cortex (IDL PFC) targeting with NIBS<sup>29,30</sup>, computational modelling using these head models will enable the development of protocols for more selective IDL PFC stimulation in this disorder. Third, EEG source localization also relies on head models to calculate the spatial location of possible current sources in the brain. Usually, boundary element models (BEM) are used which have the limitation of less anatomical detail. Therefore, finite element models (FEM) derived from high resolution MR images have become more widespread because they are able to incorporate more tissue types, increasing the precision of EEG source localization. Our head models can be used for source localization using open-source software<sup>31</sup>. Thus, our head models can help researchers to optimize NIBS protocols and EEG source localization methods, and to test them on a larger sample (including both healthy and patient data).

## Methods and results

### Participants

High-resolution head models were created from T1-weighted anatomical images that were collected in a separate functional magnetic resonance imaging (fMRI) study<sup>32</sup>. The data was obtained from the [OpenfMRI database](#) (accession number:ds000171). Structural scans of 19 healthy adult participants with no history of depression or other psychiatric disorders (11 females; mean  $\pm$  SD age: 28.79  $\pm$  10.86; range: 18–59) and 19 individuals diagnosed with MDD and experiencing a depressive episode at the time of the scanning (11 females; mean  $\pm$  SD age: 33.52  $\pm$  13.35; range: 18–56) were used. Data of one control participant ('sub-control20') was excluded due to technical problems with head model creation. Patients did not suffer from current or past manic episodes, current comorbid anxiety disorders or current alcohol dependence or abuse. At the time of data collection, all patients were unmedicated, but 6 received antidepressant pharmacotherapy in the past. For full details regarding demographic data, we refer to the supporting information of the original paper<sup>32</sup>.

### Creation of head models

As the very first step, we inspected scans of all participants, and manually removed signals corresponding to the MRI marker placed on the forehead of each subject using **FreeSurfer 5.3.0**<sup>33</sup>. Automated tissue segmentation was performed in **SPM12**<sup>34</sup> for skin, skull, eyeballs, CSF and major air cavities, and in **FreeSurfer** for gray and white matter. Subsequently, segmented images of each participant were visually inspected and manually corrected with **FreeSurfer** (done by investigator G.Cs., verified by O.P.). Manual corrections were primarily restricted to the skull-CSF boundary, but in some cases also involved the skin-skull interface. In addition, during manual corrections we verified that the segmentation of the cortical gray matter corresponded to the anatomical scans except for medial temporal lobe structures (i.e., the parahippocampal gyrus and the hippocampus proper). Moreover, the resulting masks were not corrected for inconsistencies relating to subcortical nuclei and thus, these head models are not suitable for estimating stimulation-related E-fields in structures such as the thalamus, basal ganglia, amygdala or the cerebellum. Additionally, the segmentation of the brain-stem is not accurate because it arbitrarily assigned brain tissue to white and grey matter. Furthermore, because the original dataset was de-faced and did not include the neck/shoulder region, our head models do not include these regions. This has 2 implications: Firstly, this limits their usability regarding the simulation of tDCS montages with extracephalic return electrodes. Nevertheless, they can be used for all tES protocols using scalp electrodes and most TMS protocols. Secondly, an extended head model with field of view covering the entire head would further increase the predictive accuracy of the head models<sup>35</sup>.

Head models were created with a custom version of **SimNIBS 2.1**<sup>23</sup>, a freely available software package for simulating the effects of NIBS techniques. The final head mesh of each participant consisted of a total number of approximately 3,200,000 tetrahedral elements, assigned to six tissue types (**Figure 1**). The initial segmentation included more than 6 tissue compartments (e.g., separate tissue types for cerebellar gray and white matter; available in the `m2m_sub-*` folders) but they were later combined into one of 6 tissue types: skin, skull, CSF, GM, WM and eyeballs in the final head models for simulation purposes. In addition, air cavities were modeled by not adding tetrahedra to these locations, similar to the air surrounding the head. For comparability with other datasets, we also report measurements for head size: The distance between the nasion and inion

(mean  $\pm$  SD: 19.2 cm  $\pm$  1.01 cm; range: 16.7 cm - 21.3 cm) and the distance between the right and left pre-auricular points (mean  $\pm$  SD: 14.8 cm  $\pm$  0.65 cm; range: 13.6 cm - 16.3 cm). The total volume of the brain was 1.22 dm<sup>3</sup>  $\pm$  0.11 dm<sup>3</sup> (range: 1.02 dm<sup>3</sup> - 1.49 dm<sup>3</sup>). Individual measurements are found at our data repository<sup>36</sup>.


Tissue conductivities were set as follows: 0.465 S/m (skin), 0.01 S/m (skull), 0.5 S/m (eyeballs), 1.654 S/m (cerebrospinal fluid), 0.275 S/m (gray matter), 0.126 S/m (white matter). Although our head models do not account for white matter anisotropy, this property has been shown to primarily influence current density in deeper structures, leaving superficial gray matter relatively unaffected<sup>37</sup>. The accuracy of tissue segmentation and the good correspondence between anatomical scans and the resulting head models for 8 individuals are shown in **Figure 2**.

### Dataset validation

Except for two manual steps (removal of MRI markers from the forehead, manual correction of tissue segmentations), the process of head model creation was automated using a custom version of **SimNIBS 2.1** that employed **FreeSurfer 5.3.0** for brain segmentation (as described in 38 and implemented in `mri2mesh`) and **SPM12** for segmentation of the remaining tissues (similarly to 39 and implemented in `headreco`). This pipeline provides more accurate tissue segmentation relative to other protocols. It was a custom pipeline developed before the official release of **SimNIBS 2.1**. However, using `headreco` combined with the **CAT12** toolbox (included with **SimNIBS 2.1.1**) for cortical reconstruction, the same accuracy can be achieved. We provide scripts compatible with **SimNIBS 2.1.1** for automated simulation of tDCS-induced electric fields for all head models available for download at our data repository<sup>36</sup>.


For validating the reliability of our head models, we compared the effects of two tDCS protocols targeting the IDLPFC (one conventional bipolar montage and one multi-electrode 4x1 setup) against the effects observed in the NY Head<sup>25</sup>. The mesh for the NY Head (abaqus format; <https://www.parralab.org/nyhead/>) has been reformatted to be compatible with **SimNIBS** and is also available for download in our data repository<sup>36</sup>.

For each head model, tDCS electrodes of appropriate size (bipolar montage: 5 x 5 cm, circular connectors (diameter: 0.5 cm) at the middle of the electrode pads; 4x1 montage: diameter of 1.2 cm) and thickness (1 mm for all electrodes + a sponge pocket

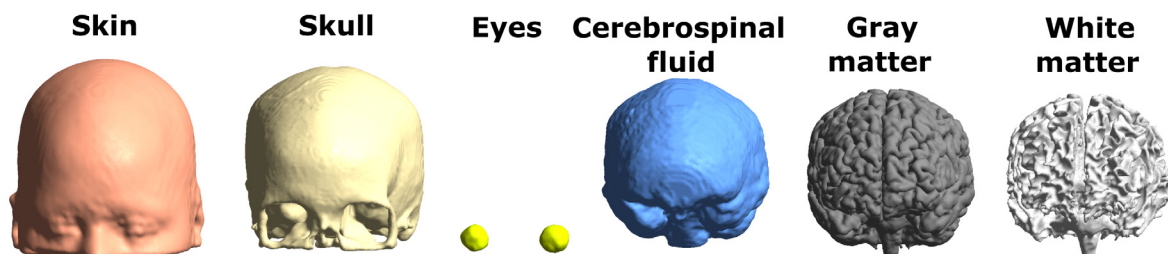

**Figure 1.** The six tissue compartments of the head models.




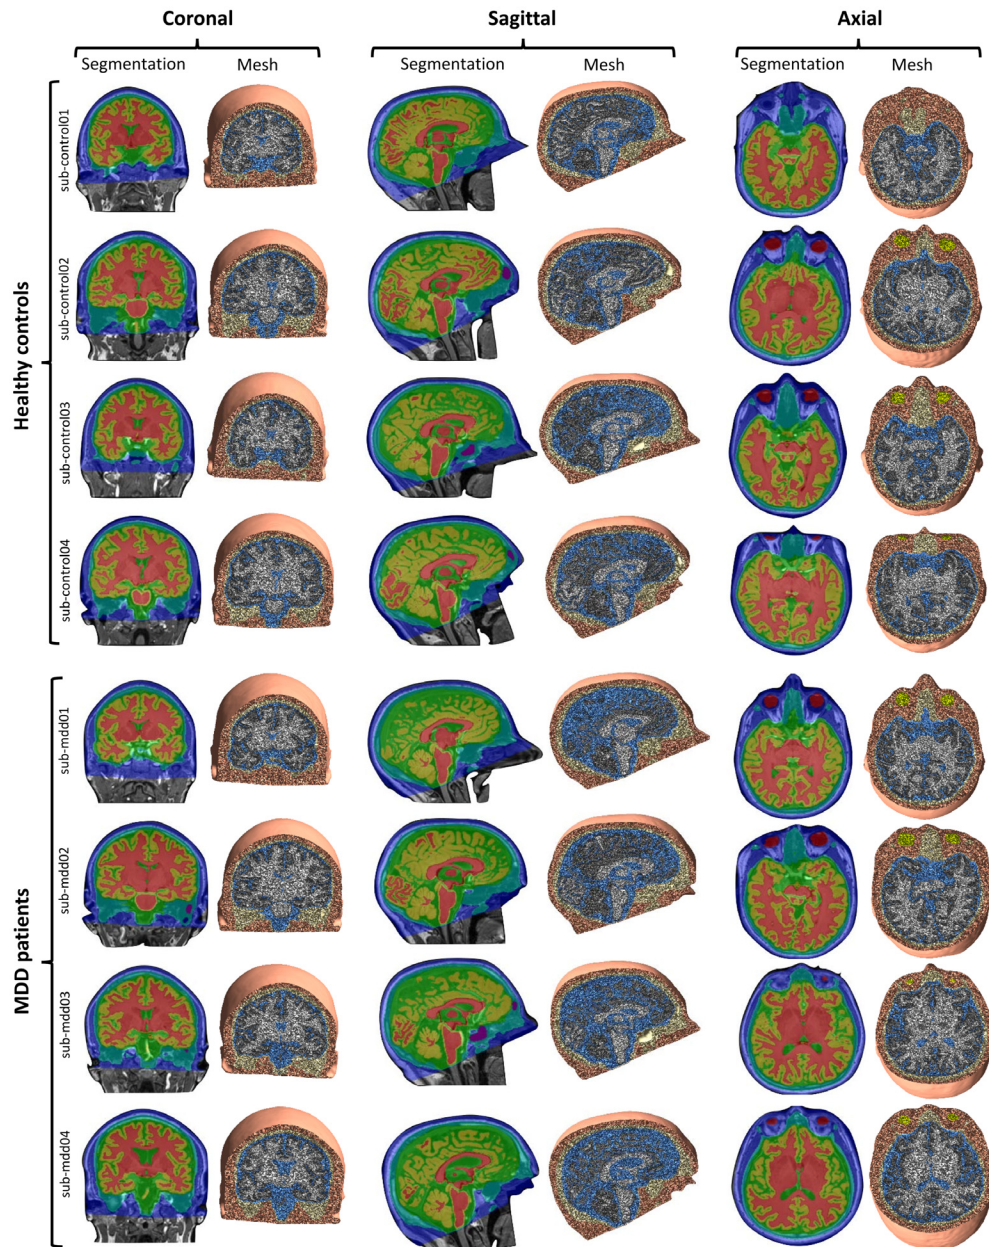

**Figure 2.** Cross-sections showing the correspondence between anatomical scans overlaid with results of the tissue segmentation (skin: dark blue; skull: turquoise; cerebrospinal fluid: green; gray matter: yellow; white matter: red; air cavities: purple, eyeballs: dark red) and the head models (meshes) for 4 individuals from both groups.

of 2.5 mm thickness for the bipolar montages and a gel layer of 2.5 mm thickness for the 4x1 montages) were placed at scalp locations corresponding to electrode positions of the International 10/10 system (bipolar montage: anode - F3, cathode - F4; 4x1 montage: anode: F3, cathodes: C3, FT7, Fp1, Fz). Stimulation intensity for the anode was set to 2 mA, with equal distribution of return currents for the 4 cathodes (0.5 mA for each) in the 4x1 protocol. Results of the simulations were visualized using Gmsh<sup>40</sup> (Figure 3).

In our previous study<sup>14</sup>, we reported stronger stimulation-induced E-fields in the IDLPFC for the bipolar montage used by Brunoni and colleagues (2013)<sup>17</sup> than for the 4x1 protocol, albeit the bipolar montage was also associated with reduced focality (i.e., more intensive stimulation of other cortical areas). Therefore, we extracted three measures for both tDCS protocols for our 38 head models: stimulation strength (the norm of the electric field vector, 'normfield') in the IDLPFC was assessed by extracting individual mean (calculated across all nodes

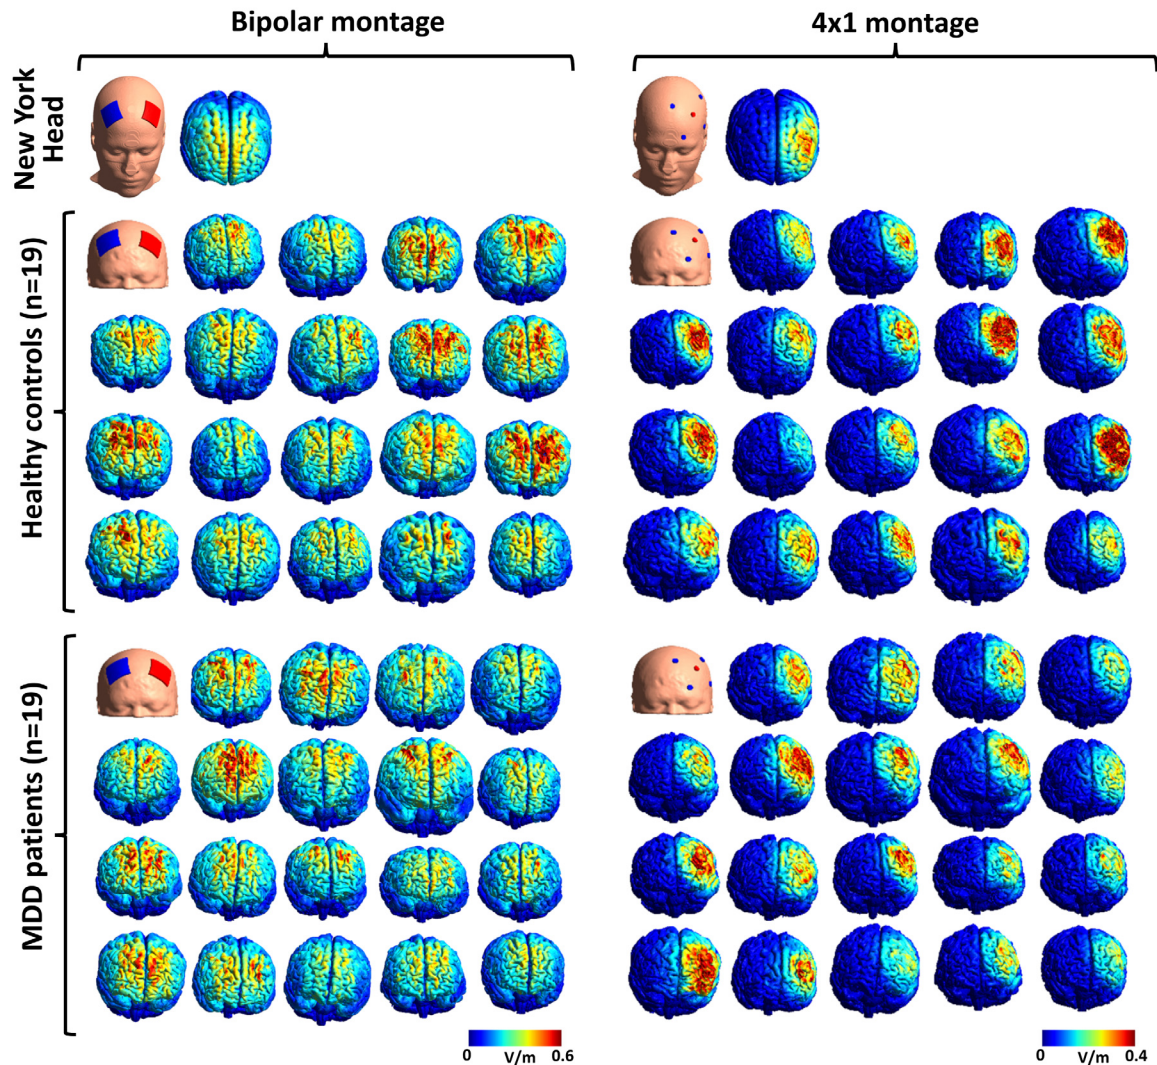


**Figure 3.** The spatial distribution of tDCS-induced E-fields in the NY Head and our 38 head models for the bipolar and the 4x1 montages. Please note the large degree of variability in E-field magnitude (both protocols) and in the lateralization of effects (bipolar protocol).

in this region) and maximum (peak) E-field values, whereas spatial focality of the stimulation was analyzed by calculating the focality-index (FI), with the target region as reference. FI was quantified as the proportion of highest-intensity nodes (nodes within the upper 1% percentile of all E-field values) in the IDLPFC relative to the whole cortex. Mean and peak E-field values corresponding to both tDCS montages were extracted by reconstructing the two-dimensional cortical surface (more precisely, the middle of the cortical sheet) of each individual along with the corresponding E-field cortical map in FreeSurfer, and an automated atlas-based parcellation of the frontal lobe<sup>41</sup> was applied to each individual brain to delineate the IDLPFC. As a result, we show that (1) both protocols induce strong E-fields in the DLPFC (with symmetrical effects for the bipolar

montage and unilateral E-field distribution for the 4x1 protocol), (2) E-field magnitudes and distributions are similar for our head models and for the NY Head, (3) all E-field measures (peak and mean strength, FI) show great degree of variability, and (4) montage-specific effects are consistent with previous results reported in the literature regarding both the spatial distribution and the magnitude of E-fields<sup>35,42–45</sup> (Figure 3, Figure 4). Accessing group differences between MDD and healthy subjects was not the primary aim of the current data note, however, analysis of the spatial distribution of tDCS-induced E-fields in the bilateral DLPFC and medial prefrontal cortex showed subtle group differences between the healthy and MDD groups. For detailed discussion of these results and that of Figure 4 we refer the reader to our accompanying paper<sup>14</sup>.



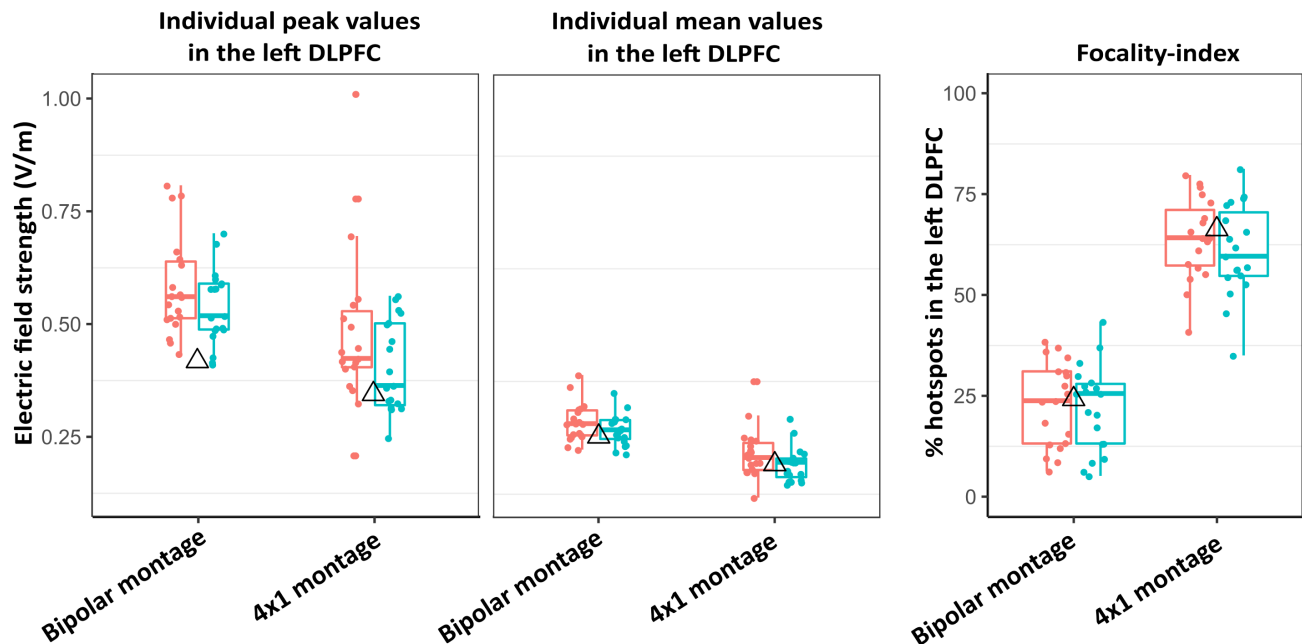

**Figure 4. Variability of tDCS-induced E-field strengths across head models for the two montages.** Both peak (left panel) and mean (middle panel) E-field magnitudes in the IDLPFC are stronger for the bipolar montage, whereas the 4x1 protocol yields more focal stimulation of the target region (right panel). Group means (red: healthy individuals, green: MDD patients) do not differ substantially, but large degree of inter-individual variability can be observed in both groups. The triangles show data for the New York Head. Horizontal lines within boxes represent median values, whereas lower and upper box hinges correspond to the first and third quartiles (25<sup>th</sup> and 75<sup>th</sup> percentiles). Lengths of upper/lower whiskers extend to the largest/smallest values that do not exceed 1.5\* the inter-quartile range; dots represent individual data.

### Data availability

*Open Science Framework (OSF)*: Dataset 1. Head models of healthy and depressed adults for simulating the effects of non-invasive brain stimulation, <http://doi.org/10.17605/OSF.IO/EXBD5><sup>36</sup>

License: CC0 1.0 Universal

At our data repository<sup>36</sup>, the following data are available for download for all subjects (healthy adults: 'sub-control', patients: 'sub-mdd'): T1-weighted anatomical scans registered to FreeSurfer conform space ('nii.gz' files), the corresponding segmentation masks for the 7 (6 tissue types of the final meshes + a mask for major air cavities) tissue types ('nii.gz' files), the final head models ('msh' files), the files containing electrode coordinates (International 10/10 system) for all participants ('txt' files) can be used for performing new script-based simulations, whereas the 'geo' files can be used to plot electrode positions directly onto the mesh files in Gmsh<sup>40</sup>, and files organized in 2 folders ('fs\_\*.tar.gz' and 'm2m\_\*.tar.gz') that enable creating simulation outputs in average FreeSurfer space ('fsaverage'). We also included a README file with a detailed description of the data and scripts.

### Usage notes

Our head models are compatible with SimNIBS 2.1.1 (<http://simnibs.de/>) for simulating the effects of tDCS and TMS protocols. This software package has an easy-to-use graphical user interface (GUI) for setting all stimulation parameters (scalp location, intensity, etc.) for both NIBS techniques. By using our

custom-written script<sup>36</sup>, it is also possible to run tDCS simulations for any given montage for all participants at once. The script will also output data registered to an average surface ('fsaverage') which allows creating group averaged data, as we have shown previously<sup>14</sup>. In addition, researchers have the opportunity to extract E-field components that are either radial (normal) or tangential relative to the cortical surface, and have been associated with different cellular effects<sup>46</sup>. At our data repository<sup>36</sup> we also provide the manually corrected segmentations for the different tissue types for those who would like to create high-quality meshes of their own using open-source software such as iso2mesh<sup>47</sup>. Finally, our meshes can be used for improving the anatomic precision of EEG source localization, using open-source tools<sup>31</sup>.

### Grant information

This work was supported by the Northern Norway Regional Health Authority (grant no. PFP1237-15) for GC and MM and by the Lundbeck foundation (grant no. R118-A11308) and the Novonordisk foundation (grant no. NNF14OC0011413) for OP and AT. The publication charges for this article have been funded by a grant from the publication fund of UiT The Arctic University of Norway.

*The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.*



## References

1. Polanía R, Nitsche MA, Ruff CC: **Studying and modifying brain function with non-invasive brain stimulation.** *Nat Neurosci.* 2018; **21**(2): 174–187.  
[PubMed Abstract](#) | [Publisher Full Text](#)
2. Bestmann S, de Berker AO, Bonaiuto J: **Understanding the behavioural consequences of noninvasive brain stimulation.** *Trends Cogn Sci.* 2015; **19**(1): 13–20.  
[PubMed Abstract](#) | [Publisher Full Text](#)
3. Stagg CJ, Nitsche MA: **Physiological basis of transcranial direct current stimulation.** *Neuroscientist.* 2011; **17**(1): 37–53.  
[PubMed Abstract](#) | [Publisher Full Text](#)
4. Antal A, Nitsche MA, Kruse W, et al.: **Direct current stimulation over v5 enhances visuomotor coordination by improving motion perception in humans.** *J Cogn Neurosci.* 2004; **16**(4): 521–527.  
[PubMed Abstract](#) | [Publisher Full Text](#)
5. Fregni F, Boggio PS, Nitsche M, et al.: **Anodal transcranial direct current stimulation of prefrontal cortex enhances working memory.** *Exp Brain Res.* 2005; **166**(1): 23–30.  
[PubMed Abstract](#) | [Publisher Full Text](#)
6. Coffman BA, Trumbo MC, Clark VP: **Enhancement of object detection with transcranial direct current stimulation is associated with increased attention.** *BMC Neurosci.* 2012; **13**(1): 108.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
7. Boggio PS, Campanhã C, Valasek CA, et al.: **Modulation of decision-making in a gambling task in older adults with transcranial direct current stimulation.** *Eur J Neurosci.* 2010; **31**(3): 593–597.  
[PubMed Abstract](#) | [Publisher Full Text](#)
8. Feeser M, Prehn K, Kazzer P, et al.: **Transcranial direct current stimulation enhances cognitive control during emotion regulation.** *Brain Stimul.* 2014; **7**(1): 105–112.  
[PubMed Abstract](#) | [Publisher Full Text](#)
9. Ridding MC, Rothwell JC: **Is there a future for therapeutic use of transcranial magnetic stimulation?** *Nat Rev Neurosci.* 2007; **8**(7): 559–67.  
[PubMed Abstract](#) | [Publisher Full Text](#)
10. Kuo MF, Paulus W, Nitsche MA: **Therapeutic effects of non-invasive brain stimulation with direct currents (tDCS) in neuropsychiatric diseases.** *NeuroImage.* 2014; **85** Pt 3: 948–960.  
[PubMed Abstract](#) | [Publisher Full Text](#)
11. Flöel A: **tDCS-enhanced motor and cognitive function in neurological diseases.** *NeuroImage.* 2014; **85** Pt 3: 934–947.  
[PubMed Abstract](#) | [Publisher Full Text](#)
12. Di Lazzaro V, Profice P, Pilato F, et al.: **Motor cortex plasticity predicts recovery in acute stroke.** *Cereb Cortex.* 2009; **20**(7): 1523–1528.  
[PubMed Abstract](#) | [Publisher Full Text](#)
13. Opitz A, Paulus W, Will S, et al.: **Determinants of the electric field during transcranial direct current stimulation.** *NeuroImage.* 2015; **109**: 140–150.  
[PubMed Abstract](#) | [Publisher Full Text](#)
14. Csifcsák G, Boayue NM, Puonti O, et al.: **Effects of transcranial direct current stimulation for treating depression: A modeling study.** *J Affect Disord.* 2018; **234**: 164–173.  
[PubMed Abstract](#) | [Publisher Full Text](#)
15. Brunoni AR, Vanderhasselt MA: **Working memory improvement with non-invasive brain stimulation of the dorsolateral prefrontal cortex: a systematic review and meta-analysis.** *Brain Cogn.* 2014; **86**: 1–9.  
[PubMed Abstract](#) | [Publisher Full Text](#)
16. Hill AT, Fitzgerald PB, Hoy KE: **Effects of anodal transcranial direct current stimulation on working memory: a systematic review and meta-analysis of findings from healthy and neuropsychiatric populations.** *Brain Stimul.* 2016; **9**(2): 197–208.  
[PubMed Abstract](#) | [Publisher Full Text](#)
17. Brunoni AR, Valiengo L, Baccaro A, et al.: **The sertraline vs. electrical current therapy for treating depression clinical study: results from a factorial, randomized, controlled trial.** *JAMA Psychiatry.* 2013; **70**(4): 383–391.  
[PubMed Abstract](#) | [Publisher Full Text](#)
18. Blumberger D, Tran L, Fitzgerald P, et al.: **A randomized double-blind sham-controlled study of transcranial direct current stimulation for treatment-resistant major depression.** *Front Psychiatry.* 2012; **3**: 74.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
19. Bennabi D, Nicolier M, Monnin J, et al.: **Pilot study of feasibility of the effect of treatment with tDCS in patients suffering from treatment-resistant depression treated with escitalopram.** *Clin Neurophysiol.* 2015; **126**(6): 1185–1189.  
[PubMed Abstract](#) | [Publisher Full Text](#)
20. Loo CK, Sachdev P, Martin D, et al.: **A double-blind, sham-controlled trial of transcranial direct current stimulation for the treatment of depression.** *Int J Neuropsychopharmacol.* 2010; **13**(1): 61–69.  
[PubMed Abstract](#) | [Publisher Full Text](#)
21. Loo CK, Alonzo A, Martin D, et al.: **Transcranial direct current stimulation for depression: 3-week, randomised, sham-controlled trial.** *Br J Psychiatry.* 2012; **200**(1): 52–59.  
[PubMed Abstract](#) | [Publisher Full Text](#)
22. Miranda PC, Lomarev M, Hallett M: **Modeling the current distribution during transcranial direct current stimulation.** *Clin Neurophysiol.* 2006; **117**(7): 1623–1629.  
[PubMed Abstract](#) | [Publisher Full Text](#)
23. Thielscher A, Antunes A, Saturnino GB: **Field modeling for transcranial magnetic stimulation: A useful tool to understand the physiological effects of TMS?** *Conf Proc IEEE Eng Med Biol Soc.* 2015; **2015**: 222–225.  
[PubMed Abstract](#) | [Publisher Full Text](#)
24. Huang Y, Datta A, Bikson M, et al.: **Realistic volumetric-approach to simulate transcranial electric stimulation—roast—a fully automated open-source pipeline.** *bioRxiv.* 2017; 217331.  
[Publisher Full Text](#)
25. Huang Y, Parra LC, Haufe S: **The New York Head-A precise standardized volume conductor model for EEG source localization and tES targeting.** *NeuroImage.* 2016; **140**: 150–162.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
26. Fonov VS, Evans AC, McKinstry RC, et al.: **Unbiased nonlinear average age-appropriate brain templates from birth to adulthood.** *NeuroImage.* 2009; **47**(Suppl 1): S102.  
[Publisher Full Text](#)
27. Fonov V, Evans AC, Botteron K, et al.: **Unbiased average age-appropriate atlases for pediatric studies.** *NeuroImage.* 2011; **54**(1): 313–327.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
28. Grabner G, Janke AL, Budge MM, et al.: **Symmetric atlas and model based segmentation: an application to the hippocampus in older adults.** *Med Image Comput Comput Assist Interv.* Springer, 2006; **9**(Pt 2): 58–66.  
[PubMed Abstract](#) | [Publisher Full Text](#)
29. Fitzgerald PB, Maller JJ, Hoy KE, et al.: **Exploring the optimal site for the localization of dorsolateral prefrontal cortex in brain stimulation experiments.** *Brain Stimul.* 2009; **2**(4): 234–237.  
[PubMed Abstract](#) | [Publisher Full Text](#)
30. De Witte S, Klooster D, Dedoncker J, et al.: **Left prefrontal neuronavigated electrode localization in tDCS: 10-20 EEG system versus MRI-guided neuronavigation.** *Psychiatry Res Neuroimaging.* 2018; **274**: 1–6.  
[PubMed Abstract](#) | [Publisher Full Text](#)
31. Ziegler E, Chellappa SL, Gaggioni G, et al.: **A finite-element reciprocity solution for EEG forward modeling with realistic individual head models.** *NeuroImage.* 2014; **103**: 542–551.  
[PubMed Abstract](#) | [Publisher Full Text](#)
32. Lepping RJ, Atchley RA, Chrysikou E, et al.: **Neural Processing of Emotional Musical and Nonmusical Stimuli in Depression.** *PLoS One.* 2016; **11**(6): e0156859.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
33. Fischl B, Sereno MI, Dale AM: **Cortical surface-based analysis. II: Inflation, flattening, and a surface-based coordinate system.** *NeuroImage.* 1999; **9**(2): 195–207.  
[PubMed Abstract](#) | [Publisher Full Text](#)
34. Friston KJ, Holmes AP, Worsley KJ, et al.: **Statistical parametric maps in functional imaging: a general linear approach.** *Hum Brain Mapp.* 1994; **2**(4): 189–210.  
[Publisher Full Text](#)
35. Huang Y, Liu AA, Lafon B, et al.: **Measurements and models of electric fields in the in vivo human brain during transcranial electric stimulation.** *eLife.* 2017; **6**: pii: e18834.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
36. Boayue NM, Csifcsák G, Puonti O, et al.: **Dataset 1. Head models of healthy and depressed adults for simulating the effects of non-invasive brain stimulation.** 2018.  
<http://www.doi.org/10.17605/OSF.IO/EXBDS>
37. Wagner S, Rampersad SM, Aydin Ü, et al.: **Investigation of tDCS volume conduction effects in a highly realistic head model.** *J Neural Eng.* 2014; **11**(1): 016002.  
[PubMed Abstract](#) | [Publisher Full Text](#)
38. Windhoff M, Opitz A, Thielscher A: **Electric field calculations in brain stimulation based on finite elements: an optimized processing pipeline for the generation and usage of accurate individual head models.** *Hum Brain Mapp.* 2013; **34**(4): 923–935.  
[PubMed Abstract](#) | [Publisher Full Text](#)
39. Nielsen JD, Madsen KH, Puonti O, et al.: **Automatic skull segmentation from MR images for realistic volume conductor models of the head: Assessment of the state-of-the-art.** *NeuroImage.* 2018; **174**: 587–598.  
[PubMed Abstract](#) | [Publisher Full Text](#)
40. Geuzaine C, Remacle JF: **Gmsh: A 3-d finite element mesh generator with built-in pre- and post-processing facilities.** *Int J Numer Meth Eng.* 2009; **79**(11): 1309–1331.  
[Publisher Full Text](#)
41. Ranta ME, Chen M, Crocetti D, et al.: **Automated MRI parcellation of the frontal lobe.** *Hum Brain Mapp.* 2014; **35**(5): 2009–2026.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
42. Bai S, Dokos S, Ho KA, et al.: **A computational modelling study of transcranial**

- direct current stimulation montages used in depression. *NeuroImage*. 2014; **87**: 332–344.  
[PubMed Abstract](#) | [Publisher Full Text](#)
43. Seibt O, Brunoni AR, Huang Y, *et al.*: **The Pursuit of DLPFC: Non-neuronavigated Methods to Target the Left Dorsolateral Pre-frontal Cortex With Symmetric Bicephalic Transcranial Direct Current Stimulation (tDCS)**. *Brain Stimul*. 2015; **8**(3): 590–602.  
[PubMed Abstract](#) | [Publisher Full Text](#)
44. Laakso I, Tanaka S, Mikkonen M, *et al.*: **Electric fields of motor and frontal tDCS in a standard brain space: A computer simulation study**. *NeuroImage*. 2016; **137**: 140–151.  
[PubMed Abstract](#) | [Publisher Full Text](#)
45. Opitz A, Falchier A, Yan CG, *et al.*: **Spatiotemporal structure of intracranial electric fields induced by transcranial electric stimulation in humans and nonhuman primates**. *Sci Rep*. 2016; **6**: 31236.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
46. Rahman A, Reato D, Arlotti M, *et al.*: **Cellular effects of acute direct current stimulation: somatic and synaptic terminal effects**. *J Physiol*. 2013; **591**(10): 2563–2578.  
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
47. Fang Q, Boas DA: **Tetrahedral mesh generation from volumetric binary and grayscale images**. In *Biomedical Imaging: From Nano to Macro, 2009. ISBI'09. IEEE International Symposium on*. Ieee, 2009; 1142–1145.  
[Publisher Full Text](#)

# Open Peer Review

## Current Referee Status:



### Version 2

Referee Report 15 November 2018

<https://doi.org/10.5256/f1000research.18435.r40676>



**Yu Huang** 

City College of New York, New York City, NY, USA

The authors have addressed all my concerns.

**Competing Interests:** No competing interests were disclosed.

**I have read this submission. I believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard.**

### Version 1

Referee Report 17 September 2018

<https://doi.org/10.5256/f1000research.16478.r37428>



**Yu Huang** 

City College of New York, New York City, NY, USA

This is a modeling effort trying to predict how electric field distributes under transcranial electric stimulation for up to 19 normal and 19 pathological subjects. It is well written and a good contribution to the literature. The authors are advised to address the following issues before indexing:

- 1) Only transcranial electric stimulation (TES) is done in this work. There is no simulation on magnetic stimulation (TMS). So the title of this manuscript should be “non-invasive *electric* brain stimulation”
- 2) The authors only discussed there are inter-individual variabilities in E-field distributions, but did not say anything about how the E-field differs (or is similar) between the healthy subjects and depression subjects, and why.
- 3) As shown in Figure 1, the head models are all cut off without the lower part of the head. This will give significant difference in the E-field distributions compared to a head model that covers the entire head (Huang and Liu, et al, 2017<sup>1</sup>). Please discuss this as one limitation of this work.
- 4) There are results in the Section Methods. So the section name should be “Methods and Results”.

- 5) It is unclear that how the IDLPFC region was separated. You only mentioned "...applying automated atlas-based parcellation of the frontal lobe to delineate the IDLPFC region in each brain". Please briefly describe how this was done. Was some atlas registered to each individual brain to extract the region?
- 6) You said SimNIBS 2.1 was used, but did not mention which function was used for the segmentation. In SimNIBS 2.1, "headreco" calls SPM12 to segment all the head tissues, and "mri2mesh" uses FreeSurfer to segment gray and white matter, and FSL to segment non-brain tissues. You said "...SimNIBS 2.1 that employed FreeSurfer 5.3.0 for brain segmentation (as described in 29) and SPM12 for segmentation of the remaining tissues (similarly to 30)." This is not clear to me. Did you combine "headreco" and "mri2mesh"? Also if you used SPM12, there should be a tissue type "air cavities", but from Figure 1, this "air cavities" is not there.
- 7) The thickness of electrodes in your models "1 mm for all electrodes + 2.5 mm sponge pocket/gel layer for the bipolar and 4x1 montages, respectively" is not clear. Please clarify this sentence.
- 8) Minor:
- In "Introduction" section, the first 3 sentences in the first paragraph are general statements but lack references. Please add.
  - In "Introduction" section, 2<sup>nd</sup> paragraph, what do you mean by "rotation or type"?

## References

1. Huang Y, Liu A, Lafon B, Friedman D, Dayan M, Wang X, Bikson M, Doyle W, Devinsky O, Parra L: Measurements and models of electric fields in the in vivo human brain during transcranial electric stimulation. *eLife*. 2017; 6. [Publisher Full Text](#)

## Is the rationale for creating the dataset(s) clearly described?

Yes

## Are the protocols appropriate and is the work technically sound?

Yes

## Are sufficient details of methods and materials provided to allow replication by others?

Partly

## Are the datasets clearly presented in a useable and accessible format?

Yes

**Competing Interests:** No competing interests were disclosed.

**I have read this submission. I believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard, however I have significant reservations, as outlined above.**

Author Response 26 Oct 2018

**Nya Boayue**, University of Tromsø, Norway



We are grateful to Dr. Huang for reviewing our manuscript. Your comments have helped give the revised version of our manuscript more clarity. We have addressed all the points raised in the new version of the MS. We have also updated the scripts at our data repository such that they are compatible with the currently released SimNIBS (version 2.1.1).

1. The title of the new manuscript has been changed based on your suggestion.
2. We chose to keep the focus here on the data since this is a data note. However, we have added the following to the **Dataset validation** section. "Accessing group differences between MDD and healthy subjects was not the primary aim of the current data note, however, analysis of the spatial distribution of tDCS-induced E-fields in the bilateral DLPFC and medial prefrontal cortex showed subtle group differences between the healthy and MDD groups. For detailed discussion of these results and that of Figure 4 we refer the reader to our accompanying paper  
<https://www.sciencedirect.com/science/article/pii/S0165032717324746>."
3. Many thanks for this very important point and pointing us to the article. This has now been addressed in our manuscript as one of the limitations of using our head models in the **creation of head models** section . "... an extended head model with field of view covering the entire head would further increase the predictive accuracy of the head models  
<https://elifesciences.org/articles/35178>"
4. The Methods section has been renamed to "Methods and Results".
5. Through personal communication with the authors of  
<https://onlinelibrary.wiley.com/doi/full/10.1002/hbm.22309>, we received a script which was used for the automatic parcellation of the frontal lobe. We have now clarified this aspect: "an automated atlas-based parcellation of the frontal lobe  
<https://onlinelibrary.wiley.com/doi/full/10.1002/hbm.22309> was applied to each individual brain to delineate the IDLPFC."
6. This is a good point. The reason for the lack of clarity is that we used a custom version of the software which, at the time, resulted in better results than using the latest released version. In the meantime, a newer SimNIBS version has been released. We have added the following detail to the MS to avoid any misunderstandings. "... the process of head model creation was automated using a custom version of SimNIBS 2.1 that employed FreeSurfer 5.3.0 for brain segmentation (as described in  
<https://onlinelibrary.wiley.com/doi/full/10.1002/hbm.21479> and implemented in mri2mesh) and SPM12 for segmentation of the remaining tissues (similarly to  
<https://www.sciencedirect.com/science/article/pii/S1053811918301800> and implemented in headreco). This pipeline provides more accurate tissue segmentation relative to other protocols. It was a custom pipeline developed before the official release of SimNIBS 2.1. However, using headreco combined with the CAT12 toolbox (included with SimNIBS 2.1.1 ) for cortical reconstruction, the same accuracy can be achieved."As for the lack of "air cavities" in the Figure 1, we have added the following clarification in the **creation of head models** section "... air cavities were modeled by not adding tetrahedra to these locations, similar to the air surrounding the head."
7. This sentence has now been clarified. It reads " 1 mm for all electrodes + a sponge pocket of 2.5 mm thickness for the bipolar montages and a gel layer of 2.5 mm thickness for the 4x1 montages."
8. We have now added the required references.
9. We meant "electrode rotation or electrode type". this has been corrected in the MS.

**Competing Interests:** No competing interests were disclosed.

Referee Report 18 June 2018

<https://doi.org/10.5256/f1000research.16478.r34789>



**Ilkka Laakso** 

Department of Electrical Engineering and Automation, Aalto University, Espoo, Finland

Non-invasive brain stimulation techniques are based on generating, either magnetically or electrically, electric fields that can alter brain neuronal activity. However, the generated electric fields can vary greatly depending on the individual anatomy of the scalp, skull and brain. This data note presents a collection of 38 individual head models (both healthy and patients) that can be used for characterisation of variability in the electric fields.

Head models were constructed from T1-weighted MRI using freely available software: FreeSurfer, SPM12 and SimNIBS. Manual verification and corrections were applied when necessary. The approach is state of art.

The datasets are provided in the Gmsh format, which can be used directly in modelling software or converted to multiple other formats using open-source software. Furthermore, raw data, including FreeSurfer subject data, are included, allowing further processing and adaptation of the data.

Minor comments:

1. In the text and Figures 1 and 2, it is written that the head models are segmented to six tissue types. Actually, it seems that there are more than six tissue compartments, as cerebellar GM and cerebellar WM are separate from the cerebral GM and WM. Also, at least some air cavities are segmented (missing from the caption of figure 2).
2. Brainstem is segmented as cerebellar white/grey matter. It may be helpful to list this as a limitation, for instance, in "Creation of head models".
3. In the abstract, sentence "... effects of non-invasive brain stimulation ...", and in "Dataset validation", sentence "The scripts used for automated simulation of tDCS effects for all head models ...". Electric fields are not "effects".

**Is the rationale for creating the dataset(s) clearly described?**

Yes

**Are the protocols appropriate and is the work technically sound?**

Yes

**Are sufficient details of methods and materials provided to allow replication by others?**

Yes

**Are the datasets clearly presented in a useable and accessible format?**

Yes

**Competing Interests:** No competing interests were disclosed.

**I have read this submission. I believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard.**

Author Response 26 Oct 2018

**Nya Boayue**, University of Tromsø, Norway

We would like to thank Dr. Laakso for reviewing our manuscript and for the helpful comments. These comments have been addressed in the new version of the manuscript. We have also updated the scripts in our data repository such that they are compatible with the currently released SimNIBS (version 2.1.1).

1. *Thanks for pointing out this issue. We have now added air cavities to the caption of Figure 2. Concerning the discrepancy between the segmentations and the final head models, we have now added the following clarification to the **creation of head models** section “The initial segmentation included more than 6 tissue compartments (e.g., separate tissue types for cerebellar gray and white matter; available in the m2m\_sub-\* folders) but they were later combined into one of 6 tissue types: skin, skull, CSF, GM, GM and eyeballs in the final head models for simulation purposes. In addition, air cavities were modeled by not adding tetrahedra to these locations, similar to the air surrounding the head.”*
2. This is an important point. We have now added the following sentence to the **creation of head models** section “Additionally, the segmentation of the brainstem is not accurate because it arbitrarily assigned brain tissue to white and grey matter.
3. We concur with this point. The abstract sentence now reads “... the electric field elicited by non-invasive brain stimulation ...” The “**Dataset validation**” sentence which was changed a bit now reads “ We provide scripts compatible with SimNIBS 2.1.1 for automated simulation of tDCS-induced electric fields for all head models ...”

**Competing Interests:** No competing interests were disclosed.

The benefits of publishing with F1000Research:

- Your article is published within days, with no editorial bias
- You can publish traditional articles, null/negative results, case reports, data notes and more
- The peer review process is transparent and collaborative
- Your article is indexed in PubMed after passing peer review
- Dedicated customer support at every stage

For pre-submission enquiries, contact [research@f1000.com](mailto:research@f1000.com)

**F1000Research**